

Series DPG-200 Digital Pressure Gage

Specifications - Installation and Operating Instructions





The Series DPG-200 Digital Pressure Gage has a precise $\pm 0.25\%$ full scale accuracy. The 4 digit digital display will reduce the potential for errors in readings by eliminating parallax error commonly produced with analog gages. The DPG-200 is packaged in a durable extruded aluminum case designed to meet NEMA 4X (IP66). The unit is powered by 12-24 VDC/VAC and contains two alarm set points along with a 4-20 mA process output. A four-button keypad allows easy access to features. These features include backlight, peak and valley, auto zero and conversion of the pressure units.

INSTALLATION

When installing gage always use 1'' hex at the base of the housing to tighten the gage to a mating fitting. Do not apply wrench to housing.

WIRING



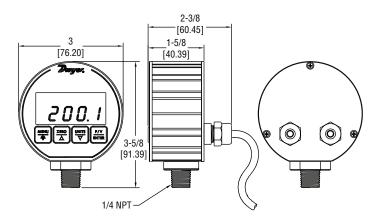

SPECIFICATIONS

DIGITAL GAGE SPECIFICATIONS

Service: Liquids and non-combustible compatible gases. Wetted Materials: Type 316L SS. Housing: Black polycarbonate front & back cover, anodized aluminum extruded housing with recessed grooves, polycarbonate overlay, Buna-N O-rings, 316L SS sensor construction. Accuracy: 0.25% F.S. ±1 least significant digit. (Includes linearity, hysteresis, repeatability). Pressure Limit: 2x pressure range for models 1000 psi; 5000 psi for 3000 psi range; 7500 psi for 5000 psi range. Temperature Limits: 0 to 158°F (0 to 70°C). Process Connection: 1/4" male NPT. Display: 4 digit (.425 H x .234 W digits). Size: 3.00" OD x 1.90 deep (not including cables). Weight: 8.84 oz (275 g).

SWITCH SPECIFICATIONS

Switch Type: 2 SPDT Form C contacts.
Electrical Rating: 0.5A @ 125 VAC resistive, 1A @ 24 VDC.
Relay Differential: 1 least significant digit.
Electrical Connections: Two 3 ft (.91 m) cables.
Mounting Orientation: Mount in any position.
Set Point Adjustment: Via menu.

TRANSMITTER SPECIFICATIONS

Temperature Limits: 0 to $158^{\circ}F$ (0 to $70^{\circ}C$). Thermal Effect: Between 70 to $158^{\circ}F = 0.016\%/^{\circ}F$. Between 0 to $70^{\circ}F = 0.026\%/^{\circ}F$. Power Requirements: 12 to 24 VAC ±20% 50 to 400 HZ, 12 to 24 VDC ±20%. Output Signal: 4 to 20 mA. Loop Resistance: 600 ohms maximum. Power Consumption: 0.8 W max. Electrical Connections: 2 three foot cables.

Enclosure Rating: Designed to meet NEMA 4X (IP66).

WARNING: DO NOT pressurize DPG over maximum allowable pressure limits. Extreme damage can occur if limits are exceeded (see Pressure Limit under Specifications). An overflow "OFL" designator will flash to acknowledge that the gages pressure range has been exceeded.

HOME


- Top line shows units.
- Bottom line shows pressure.
- If pressure is 1% F.S. below range of instrument the pressure value will alternate UFL on a 1 second interval.
- If pressure is 1% F.S. above range of instrument the pressure value will alternate with DFL on a 1 second interval.
- · Factory set to PSI.

BUTTON OPERATION


15

ENU 🔶 See menu page.

■ _> Zeros display if within ±4% F.S. of zero.



PEAK VALLEY

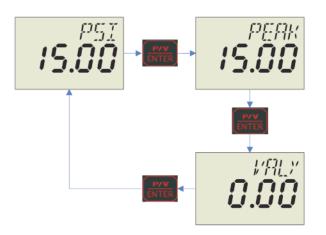

PEAK

- Highest pressure since peak and valley was reset.
- Zero button resets both peak and valley to the current pressure.


VALLEY

Lowest pressure since peak and valley was reset.
 Zero button resets both peak and valley to the current pressure.

Units Chart

| | Range | Pressure Ranges | | | | | | | | | | |
|---------|----------|--------------------|--------|--------|--------|--------|--------|--------------------|--------|-------|-------|--------|
| Model | psi | kg/cm ² | bar | in Hg | ft wc | ft sw* | kPa | oz/in ² | in wc | mbar | cm wc | mm Hg |
| DPG-200 | -14.70-0 | -1.033 | -1.013 | -29.93 | -33.94 | -33.06 | -101.4 | -235.2 | -407.3 | -1013 | -1034 | -760.7 |
| DPG-202 | 15.00 | 1.055 | 1.034 | 30.54 | 34.61 | 33.73 | 103.4 | 240 | 415.2 | 1034 | 1055 | 775.7 |
| DPG-203 | 30.00 | 2.109 | 2.069 | 61.08 | 69.21 | 67.45 | 206.9 | 480 | 830.4 | 2069 | 2109 | 1551 |
| DPG-204 | 50.00 | 3.515 | 3.448 | 101.8 | 115.4 | 112.4 | 344.8 | 800 | 1384 | 3448 | 3515 | 2586 |
| DPG-205 | 100.0 | 7.03 | 6.895 | 203.6 | 230.7 | 224.8 | 689.5 | 1600 | 2768 | 6895 | 7031 | 5172 |
| DPG-206 | 200.0 | 14.06 | 13.79 | 407.2 | 461.4 | 449.7 | 1379 | 3200 | 5536 | | | |
| DPG-207 | 300.0 | 21.09 | 20.69 | 610.8 | 692.1 | 674.5 | 2069 | 4800 | 8304 | | | |
| DPG-208 | 500.0 | 35.15 | 34.48 | 1018 | 1154 | 1124 | 3448 | 8000 | | | | |
| DPG-209 | 1000 | 70.3 | 68.98 | 2036 | 2307 | 2248 | 6895 | | | | | |
| DPG-210 | 3000 | 210.9 | 206.9 | 6108 | 6921 | 6745 | | | | | | |
| DPG-211 | 5000 | 351.5 | 344.8 | | | | | | | | | |

Compound Ranges Available: DPG-220 Range: 30" Hg-0-15 psi; DPG-221 Range: 30" Hg-0-30 psi; DPG-222* Range: 30" Hg-0-45 psi; DPG-223*: Range 30" Hg-0-60 psi; DPG-224: 30" Hg-0-100 psi. *feet of seawater @ 4°C

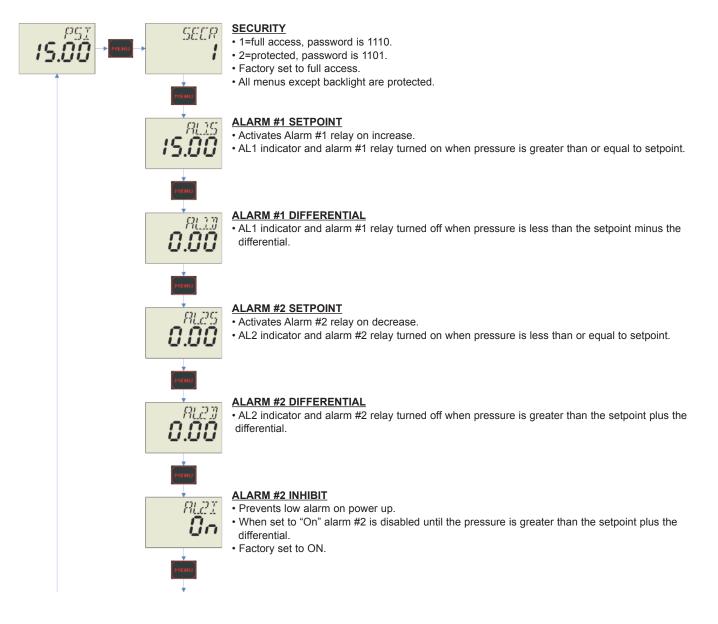

MENU BUTTON OPERATION



Advances menu. Hold for 1 second to go back to home page.



Increases value – top line of display begins to blink. Hold for 1 second to increase fast.




Decreases value – top line of display begins to blink. Hold for 1 second to decrease fast.



Stores value – top line of display stops blinking. If menu pressed before enter button pressed the value is lost.

MENU CONTINUED

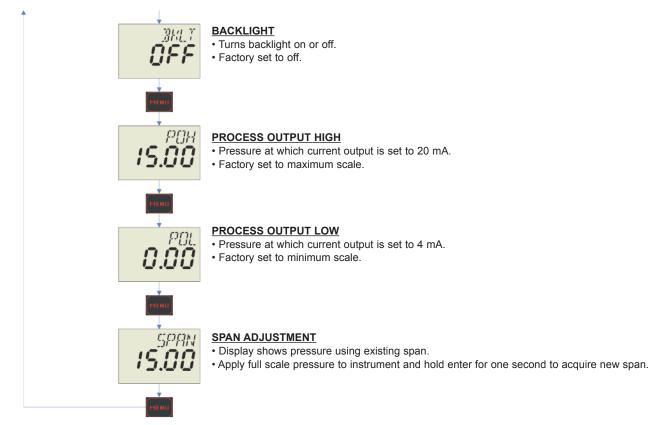

MENU BUTTON OPERATION



Advances menu. Hold for 1 second to go back to home page.

Alarm 1



Increases value – top line of display begins to blink. Hold for 1 second to increase fast.




Decreases value – top line of display begins to blink. Hold for 1 second to decrease fast.



Stores value – top line of display stops blinking. If menu pressed before enter button pressed the value is lost.

ALARM OPERATION



PRESSURE 20-(psi) 0 40-(psi) 20-10-0 412S + AL2D AL2D AL2D AL2D AL2D AL2D TIME

RL15 sets the relay on point, and RL15 - RL10 sets the relay off point. The relay's output functions in the direct acting mode, which means the relay activates with an increase in pressure. In the above graph, an instrument with a 50 psi range has the RL15 set at 40. The relay will turn on at 40 psi increase. The RL10 is set at 30. The relay will turn off at 10 psi decrease (40 - 30 = 10).

RL25 sets the relay on point, and RL25 + RL20 sets the relay off point. The relay's output functions in the reverse acting mode, which means the relay activates with a decrease in pressure. In the above graph, an instrument with a 50 psi range has the AL2S relay turn on at 10 psi decrease. The RL20 is set at 30. The relay will turn off at 40 psi increase (10 + 30 = 40).

©Copyright 2013 Dwyer Instruments, Inc.

DWYER INSTRUMENTS, INC. P.O. Box 373 • Michigan City, IN 46360, U.S.A. Printed in U.S.A. 2/13

FR# 18-443202-30 Rev. 1

Phone: 219/879-8000 Fax: 219/872-9057 www.dwyer-inst.com e-mail: info@dwyer-inst.com